



# **iJRASET**

International Journal For Research in  
Applied Science and Engineering Technology



---

# **INTERNATIONAL JOURNAL FOR RESEARCH**

IN APPLIED SCIENCE & ENGINEERING TECHNOLOGY

---

**Volume: 6**

**Issue: X**

**Month of publication: October 2018**

**DOI:**

**[www.ijraset.com](http://www.ijraset.com)**

**Call:  08813907089**

**E-mail ID: [ijraset@gmail.com](mailto:ijraset@gmail.com)**

# Utilization of Steel Slag as Partial Replacement of Cement in Concrete Pavement

Ankush Kataria<sup>1</sup>, Sonia<sup>2</sup>, Rakhi<sup>3</sup>, Sonia<sup>4</sup>

<sup>1, 2, 3, 4</sup> Student M.tech, Civil Engineering (H.S.E.), DCRUST, Murthal, Sonapat, Haryana, India

**Abstract:** This experimental work attempts to identify the behaviour of M35 grade of concrete by partial replacement of cement (OPC 43) by STEEL SLAG. In this work steel slag is used as a replacing agent to reduce the usage of cement. With this the CO<sub>2</sub> emitted during the manufacturing of cement can be reduced to a certain level. This will be advantageous to the environment as there will be reduction of green house gases. This experimental work is carried out in 5 phases in which M35 grade of concrete is prepared. 1<sup>st</sup> phase (0% steel slag + 100% cement), 2<sup>nd</sup> phase (10% steel slag + 90% cement), 3<sup>rd</sup> phase (20% steel slag + 80% cement), 4<sup>th</sup> phase (30% steel slag + 70% cement), 5<sup>th</sup> phase (40% steel slag + 60% cement). The cube mould of size 150mm X 150mm X 150mm is used for testing of compressive strength of concrete and the beam mould of size 150mm X 150mm X 700mm is used for testing of flexural strength of concrete.

**Keywords:** Cement, Steel Slag, Compressive Strength, Flexural Strength

## I. INTRODUCTION

The steel slag is a by-product of steel industry. It is produced during the production of steel. Electric arc furnace process is the process during which steel slag is obtained. In this process high power electric arc are used in the furnace to produce the heat which is required to melt the steel scrap and to convert it into high quality steel. The graphite electrode with the spout are provided in the electric arc furnace. The electric arc resists the electric flow which generates the heat at a very high temperature but the scrap metal could not resist the electricity and the scrap starts melting and in some time all the scrap changes into the molten state. This process can take up to 3 hours to complete. The temperature of electric arc furnace can reach up to 1800°C.

TABLE-I  
PHYSICAL PROPERTIES OF STEEL SLAG

Test	Results
Specific gravity	3.4
Unit weight	1782 kg/m <sup>3</sup>
Water absorption	1.6 %

TABLE-II  
CHEMICAL PROPERTIES OF STEEL SLAG

Chemical	Percentage (%) by mass
Silica	32.48
Alumina	9.83
Lime	39.42
Iron oxide	0.93
Magnesia	11.67
Sodium oxide	0.13
Potassium oxide	0.28
Sulphate	1.79
Loss of ignition	2.18

## II. METHODOLOGY

### A. Collection of Materials

- 1) Cement
- 2) Sand
- 3) Coarse aggregate
- 4) Water
- 5) Steel Slag
- 6) Admixture

The above materials were collected from the nearest material supplier except steel slag which was collected from Shree Durga Steel Industries Pvt. Ltd. Situated in village-Bhalgarh, district-Sonapat, Haryana

Shree cement OPC 43 grade was used

Admixture – FORSOC Conplast SP430 ES2 was used.

### B. Testing of Materials

TABLE-III  
TEST RESULTS FOR CEMENT OPC 43 GRADE

Specific gravity	3.17
Consistency of cement	32
Initial setting time	46 minutes
Final setting time	244 minutes
Compressive strength 3 days	24.10 N/mm <sup>2</sup>
Compressive strength 7 days	36 N/mm <sup>2</sup>
Compressive strength 14 days	44.60 N/mm <sup>2</sup>

TABLE-IV  
TEST RESULTS FOR SAND

Specific gravity	2.69
Water absorption	0.8%
Sieve analysis	Zone II

TABLE-V  
TEST RESULTS FOR COARSE AGGREGATE ( 10mm & 20mm)

Tests	10 mm	20 mm
Specific gravity	2.615	2.648
Water absorption	0.5%	1.2%

### C. Mix design

Test data

- Grade designation – M35
- Type of cement – OPC 43 grade
- Minimum cement content – 325 kg/ m<sup>3</sup>
- Maximum W/C ratio – 0.45
- Workability (slump) – 25 to 50mm
- Specific gravity of cement – 3.17
- Specific gravity of 20mm aggregate – 2.648
- Specific gravity of 10mm aggregate – 2.615
- Specific gravity of fine aggregate – 2.69
- Admixture –FORSOC Conplast SP430 ES2

Admixture ratio – 0.7% of cement content by weight  
 Sieve analysis of fine aggregate – conforming to Zone II (IS 383-1970)

1) Design Mix Calculations

$$\begin{aligned} \text{Target strength } f'_{ck} &= f_{ck} + 1.65 \times s \\ &= 35 + 1.65 \times 5 \\ &= 43.25 \text{ N/mm}^2 \end{aligned}$$

$$\text{W/C ratio} = 0.42 \text{ (for workability of 25- 50 mm)}$$

$$\text{Maximum Water content for 20 mm aggregates} = 186 \text{ Kg/ m}^3$$

$$\begin{aligned} \text{Cement Content} &= 186 / 0.42 \\ &= 443 \text{ Kg/ m}^3 \end{aligned}$$

$$\text{Volume of Coarse aggregates 20mm} = 0.619$$

$$\text{Volume of Fine aggregates} = 1 - 0.619 = 0.381$$

Mix Calculations:-

$$\text{Volume of Concrete} = 1 \text{ m}^3$$

$$\begin{aligned} \text{Volume of cement} &= (443/3.16) \times (1/1000) \\ &= 0.140 \text{ m}^3 \end{aligned}$$

$$\begin{aligned} \text{Volume of water} &= (186/1) \times (1/1000) \\ &= 0.186 \text{ m}^3 \end{aligned}$$

$$\begin{aligned} \text{Volume of all in aggregates} &= (a - (b + c)) \\ &= [1 - (0.140 + 0.186)] \\ &= 1 - 0.326 \\ &= 0.674 \text{ m}^3 \end{aligned}$$

$$\begin{aligned} \text{Mass of Coarse aggregate} &= 0.674 \times 0.619 \times 2.64 \times 1000 \\ &= 1102 \text{ kg/m}^3 \end{aligned}$$

$$\begin{aligned} \text{Mass of the Fine aggregates} &= 0.674 \times 0.381 \times 2.69 \times 1000 \\ &= 691 \text{ kg/m}^3 \end{aligned}$$

So,	W/C ratio	= 0.42		
	Cement	= 443 Kg/m <sup>3</sup>	= 443/443	= 1
	Fine aggregates	= 691 kg/m <sup>3</sup>	= 691/443	= 1.55
	Coarse aggregates	= 1102 kg/m <sup>3</sup>	= 1102/443	= 2.487
	Water	= 186 kg/m <sup>3</sup>		
	Admixture	= 0.7% of cement content by weight		

$$\text{RATIO} = 1 : 1.55 : 2.487$$

D. Mixing Process

The weight of all the material are measured sapeerately using weighing machine and the mixing machine is used for the mixing process

E. Moulding and Demoulding Process

The prepared concrete is filled into the cube moulds of size 150mm x 150mm x150mm and the beam mould of size 150mm x 150mm x 700mm. Proper compaction of the concrete is ensured by using vibration machine for the removal of air voids in the concrete mix, the vibration machine is used for the time of two minutes.

The cube moulds are demoulded after 24 hour and the beam moulds are demoulded after 48 hours.

F. Curing Process

After removing of the moulds the cubes and the beams specimens are placed in the tank filled with water in the laboratory till the date of testing.

G. Testing Process

The cube moulds for compressive strength are tested for 7 days, 14 days and 28 days and the beam moulds for flexural strength are tested for 7 days and 28 days.

H. Test Results

TABLE-VI  
Test Results For Compressive Strength Of Cubes

Mix proportion	7 days (mpa)	14 days (mpa)	28 days (mpa)
0% steel slag	16.07	29.92	44.65
10% steel slag	16.57	29.55	44.45
20% steel slag	16.26	31.12	46.45
30% steel slag	19.14	33.02	47.85
40% steel slag	14.82	28.37	42.37

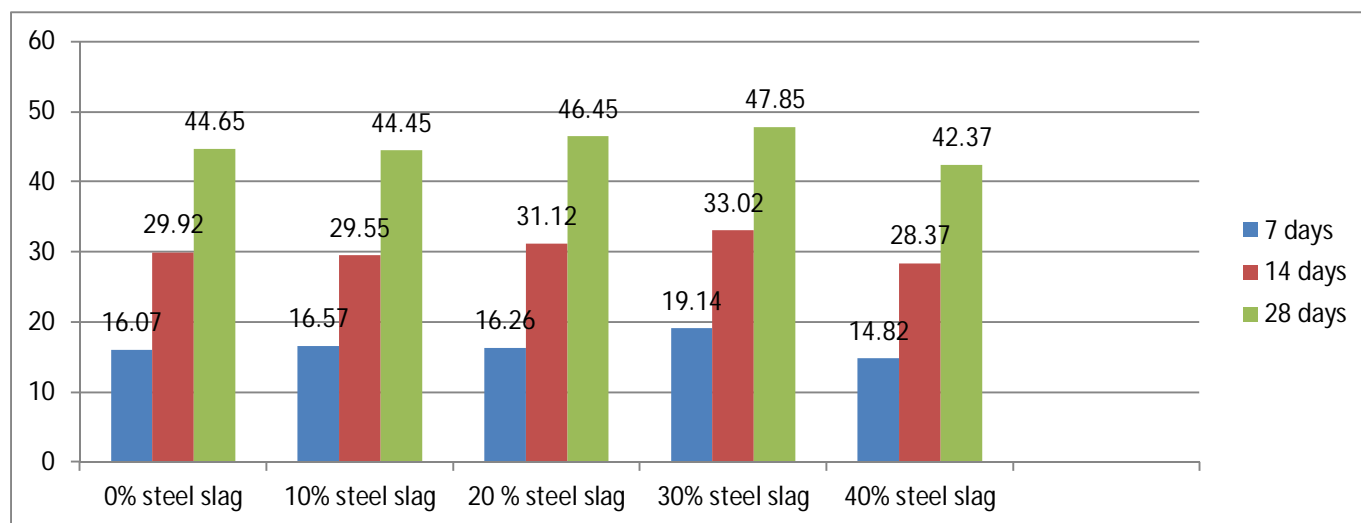


Figure 1-Compressive Strength values of cubes

TABLE-VII  
Test Results for Flexural Strength Of Cubes

Mix %	7 days	28 Days
0% steel slag	3.13	4.82
10% steel slag	3.26	5.03
20% steel slag	3.65	5.63
30% steel slag	2.89	4.45
40% steel slag	2.85	4.39

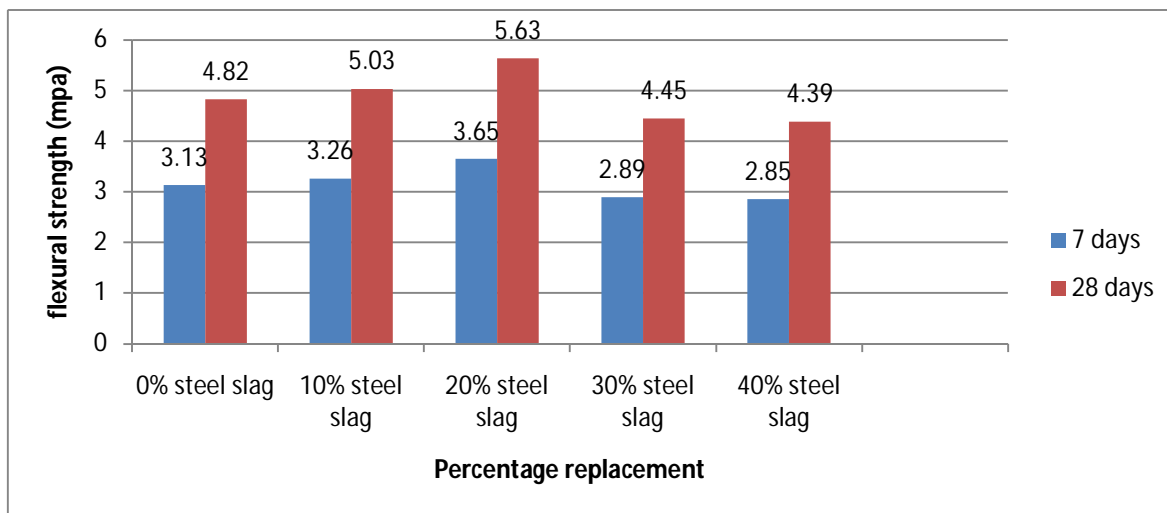


Figure 2 - Flexural Strength values of beams

### III. CONCLUSION

- 1) The workability of concrete decreases with the increase in steel slag, the particles of steel slag reduces the amount of water required to produce a given slump.
- 2) The compressive strength and flexural strength increases with the increase of steel slag in concrete up to 30%. Replacement with cement in conventional mix, however the compressive strength increases more as compared to flexural strength, the values are acceptable as per IRC.
- 3) As per results optimum percentage of steel slag for compressive strength is 30%. At 30% replacement of steel slag with cement for M35 grade concrete compressive strength is maximum. For flexural strength optimum percentage for replacement of cement with steel slag is 20%.
- 4) Mixing of steel slag in concrete conventional mix has resulted in considerable variation in the properties of fresh concrete. Integration of fly ash in concrete increased the cohesiveness of the mix, prohibited segregation and resulted in reduced bleeding. Higher percentages of steel slag can cause a change in color of the mix.

### REFERENCES

- [1] Shetty, M.S., "Concrete Technology", 4 th edition, S. Chand & Company, New Delhi, 2005.
- [2] Maslehuddin, S. M., Alfarabi, S. M., Ibrahim, M., Barry, M., "Comparison of properties of steel slag and crushed limestone aggregate concrete", Construction and Building Materials, Vo.1 17, Issue 2, pp 105-112, 2003.
- [3] Isa, Y., Omer, O.,Turhan, B., Use of GBFS in concrete as fine aggregate, Materials Journal, Vol. 103, Issue 3, pp 203-208, 2006.
- [4] JLI Yun-feng, YAO Yan, WANG Ling – "Recycling of Industrial Waste and Performance of Steel Slag green concrete"- J.Cent.SouthUniv.Technol(2009) 16:0768-0773,2009.
- [5] Ziauddin A. Khan1 , Rezqallah H. Malkawi2 , Khalaf A. Al-Ofi3 , and Nafisullah Khan4 - Review of Steel Slag Utilization in Saudi Arabia -The 6th Saudi Engineering Conference, KFUPM, Dhahran, December 2002-vol. 3. 369
- [6] 1.Qiang Wang, Peiyu Yan, Jianwen Feng ( 2010 ), A discussion on improving hydration activity of steel slag by altering its mineral compositions, Journal of Hazardous Materials , Issue 186, pp. 1070–1075
- [7] Perviz Ahmedzade, Burak Sengoz (2009), Evaluation of steel slag coarse aggregate in hot mix asphalt concrete, Journal of Hazardous Materials, Volume 165, Issues 1–3, 15 June 2009, pp. 300- 305.
- [8] Khajuria Chetan, Rafat Siddique, (June,2014) "Use of Iron Slag as Partial Replacement of Sand to Concrete", International Journal of Science, Engineering and Technology Research (IJSETR), Volume 3, Issue 1877ISSN: 2278 – 7798, p.p 1877-1880.
- [9] Ansu John and Elson Johne (2015)-Study on the partial replacement of fine aggregate using induction furnace slag. ISSN : 2320-0847 p-ISSN : 2320 0936 Volume-4 pp-01-05.
- [10] G.Ravi Vol. 05, Issue 05 (May. 2015), ||V3|| PP 64-73Experimental Investigation Of Coarse Aggregate With Steel Slag In Concrete
- [11] Prasanna Krishna P, Venkata Kiranmayi K. (2016) "Steel Slag as a Substitute for Fine Aggregate in High Strength Concrete", International Journal of Engineering Research & Technology (IJERT), ISSN: 2278-0181, p.p 810- 814.



10.22214/IJRASET



45.98



IMPACT FACTOR:  
7.129



IMPACT FACTOR:  
7.429



# INTERNATIONAL JOURNAL FOR RESEARCH

IN APPLIED SCIENCE & ENGINEERING TECHNOLOGY

Call : 08813907089  (24\*7 Support on Whatsapp)