



IJRASET

International Journal For Research in
Applied Science and Engineering Technology



INTERNATIONAL JOURNAL FOR RESEARCH

IN APPLIED SCIENCE & ENGINEERING TECHNOLOGY

Volume: 3 Issue: VI Month of publication: June 2015

DOI:

www.ijraset.com

Call:  08813907089

E-mail ID: ijraset@gmail.com

A Review on Micro Electronic Pill

Mrs. Shital Baghel¹, Nikhil Kumar Yadav²

*M.Tech (Electronics & Communication Scholar), Indian Institute Of Technology, Kharagpur
M.Tech (Power System Engineering Scholar), Dr. C.V. Raman University Bilaspur, Chhattisgarh India*

Abstract: - *The purpose of this paper is to provide the information about the innovation of new device called Micro Electronic Pill in the field of Bio-Medical Measurement, this is mainly used for diagnosis of internal part mainly gastrointestinal system which cannot be easily done with the help of normal endoscope. It is modern wireless type of endoscopic monitoring system.*

I. INTRODUCTION

The microelectronic pill is a small capsule shaped electronic pill that can be comfortably swallowed by any normal patient. It consists of lens, antenna, transmitters, camera or sensors and battery. It can reach regions such as small intestine and provides the video wirelessly to the receiving device connected to the monitoring system outside the human body and kept at distance of 1 meter. The transmission of data takes place through the radio communication between electronic pill transmitter and external receiver. Parameters such as temperature, pH and pressure of gastrointestinal tract can be measured, for the detection of diseases and disturbance in gastro intestinal system which prevents the entry of conventional endoscopic tube, a micro pill with single channel radio telemetric function is preferred. The invention of semiconductors provides ease in development of concise electronic pill capable to carry and transmit huge amount of data at a time without affecting the human body. The diagram below represents the wireless video transmission between transmitter and receiver:

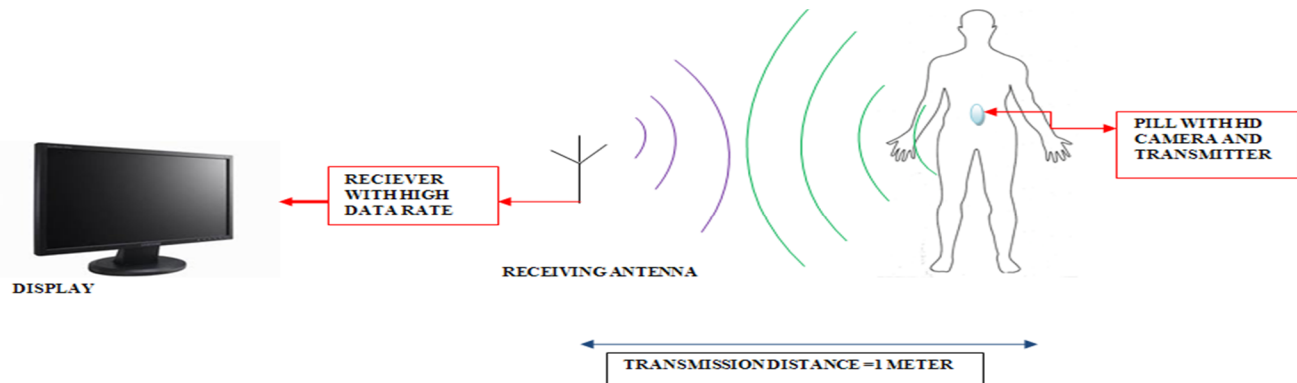


Fig 1:- Wireless Endoscope through Micro Electronic Pill

II. CONSTRUCTION

A Microelectronic pill construction requires narrow band transmission and has limited camera pixels. One of the commercially available endoscopic devices designed by the company "Given Imaging" uses Radio Frequency chip for wireless communication for real time video transmission based on the Medical Implant Communication Service band. The channel bandwidth allowable for this band is limited to 300 kHz; the low frequency application provides high transmission efficiency through layers of skin. It is very much difficult to carry enough data rate for high definition real time video data during real time monitoring process. So, for better real time diagnosis there is requirement of higher bandwidth data transmission. The fabrication of sensors of electronic pill are done on two silicon chips which is generally kept at the top of the capsule and the first chip encompasses diode, the pH ISFET sensor, temperature sensor and conductivity sensor with two sensor. The another chip has thermometer and oxygen sensor.

The method which provides the baud rate of 100Mbps is Wideband Technology. This technology is currently used in radar, Image processing and In-door entertainment. But, the major problem in high frequency is the major loss in

International Journal for Research in Applied Science & Engineering Technology (IJRASET)

body tissue. The schematic diagram of pill is represented by the figure below:-

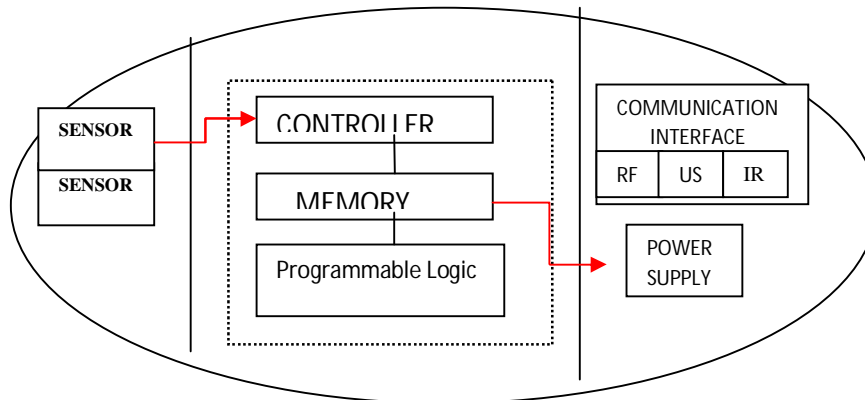


Fig: 2- BLOCK DIAGRAM OF SWALLOWABLE MICRO ELECTRONIC PILL

III. DESCRIPTION

All Microelectronic pill is powered by a battery, in order to utilize the device in internal remote locations. There is scanning receiver which captures the wireless radio signal from pill through a coil antenna. A computer system is required for the control of data acquisition unit which acquires data in analog form from the scanning receiver. It provides recording of data on the computer. Stable transmission frequency must be constantly maintained. The transmission frequency is measured with the help of change in temperature. The change in frequency is measured with the help of scanning receiver, and the result obtained is used to evaluate the advantage of crystal stabilized unit.

The power consumption of microelectronic including transmitter and sensors connected is calculated to 12.1 milliwatt with current rating 3.9mill Ampere at 3.1 volt voltage supply, where as free running radio transmitter consumes 6.8milliwatt. Two silver oxide batteries SR44 are used to provide operating time of more than 40 hours. The pH measurement ranges from 1 to 13 can be carried out. The dissolved oxygen is up to 8.2 mg per liter. The temperature measurement is done from 0°C to 70°C. The pH ISFET sensor operated in constant current mode, with the drain voltage connected to the positive supply and the source voltage changes as per gate potential and gate potential is grounded. In control chip, the noise from application specific integrated circuit provides a constant level of 3Mega volt peak to peak, which provides single Least Significant Bit of Analog to Digital Converter; the second Least Significant Bit is used to provide an adequate noise margin, and here to have an effective resolution of 8 bits the 10-bit Analog to Digital Converter is used.

The components of capsule must be capable to protect itself from corrosive environment in gastro intestinal tract and it must be non-toxic to the human being but as the battery electrodes are toxic in nature, so care must be taken to prevent leakage of toxic fluids into the digestive system.

IV. ADVANTAGES

- A. It is beneficial to detect the diseases and malfunctioning in the remote areas of gastro intestinal tract just like pancreatic disease, inflammatory bowel disease, activity of fermented bacteria, acidic level and oesophagus reflux which is out of reach for conventional endoscopic device.
- B. It can be used in corrosive surrounding of GI tract.
- C. It consumes very less power as it operates in Programmable Standby Mode.
- D. Its practical application is very simple as it has very small in size.
- E. The battery lasts for 40 hours which is sufficient to carry out any type of complete internal diagnosis.
- F. The transmission length is limited to a distance of only one meter, so it has zero noise interference.

V. DISADVANTAGES

- A. The ultrasonic activities and impedance topographies cannot be performed by this.

International Journal for Research in Applied Science & Engineering Technology (IJRASET)

- B. It is unable to detect radiation abnormalities.
- C. The treatment through Micro Pill is very expensive and is not available in many regions.
- D. The size of pill is small but it is not as small that can be digested by small babies.

VI. SUMMARY

Human body is very sensitive even for small changes. Many times the doctors fail to interpret the diseases and abnormalities which make the curing of diseases more difficult, so the Micro Electronic pill is developed by the scientists to overcome from this problem and quick diagnosis is possible by this innovation. To carry out above process efficiently a radio system of high capacity is needed for this technology to get real time video of digestive system wirelessly, this requires Upper Wide Bandwidth Transmitter and Receiver. But tissue damage at high frequency limited its usage. Research work is carried out to get the detailed images of internal parts through high frequency transmission and reception of data without damage to tissues of human body.

REFERENCES

- [1] R. S. Mackay, "Endpradiosonde," *Nature* vol. 179, 1957
- [2] G. Meron, "The development of the swallowable video capsule (M2A)," *Gastrointestinal Endoscopy*, vol. 6, pp. 817-8199, 2000.
- [3] M. Q. H. Meng, et al., "Wireless Robotic Capsule Endoscopy: State-of the Art and Challenges," in the 5th World Congress on intelligent Control and Automation, 2004, vol. 6, pp. 5561-5565.
- [4] <http://www.givenimaging.com/>, 2009.
- [5] P. Bradley, "An ultra low power, high performance medical implant communication system (MICS) transceiver for implantable devices," in the IEEE Biomed. Circuits and Systems Conference, pp. 158-16, 2006.
- [6] J. Nagumo et al., "Echo capsule for medical use," *IRE Transaction on Bio-medical Electronics*, vol. 9., pp. 195-199, 1962.
- [7] C. Mc Caffrey, et al. "Swallowable-capsule technology," *Pervasive computing*, January-March, 2008.
- [8] V. K. Zworykin, "Radio pill," *Nature*, vol. 179, p. 898, 1957.
- [9] R. S. Mackay and B. Jacobson, "Radio telemetering from within the human body," *Science*, vol. 134, pp. 1196-1202, 1961.
- [10] X. Chen et al. "A wireless capsule endoscope system with low-power controlling and processing ASIC," *IEEE Transation on Biomedical Circuits and Systems*, Vol. 3, February 2009.
- [11] E. A. Johannessen, et al. "Biocompatibility of a lab-on-a-pill sensor in artificial gastrointestinal environments," *IEEE Trans. Biomed. Eng.*, vol. 53, pp. 2333, Nov. 2006.
- [12] P. Valdastrì, A. Menciassi, A. Arena, C. Caccamo and P. Dario "An implantable telemetry platform system for in vivo monitoring of physiological parameters," *IEEE Trans. Inform. Technol. Biomed.*, vol.8, pp. 271, Sep. 2004.
- [13] K. Wang, G. Yan, P. Jiang, and D. Ye, "A wireless robotic endoscope for Gastrointestine," *IEEE Trans. Robotics*, Vol.24, pp. 206-210, February 2008.
- [14] J. Thone, S. Radiom, D. Turgis, R. Carta, G. Gielen, and R. Puers, "Design of a 2 Mbps FSK near-field transmitter for wireless capsule endoscopy," *Sensors and Actuators A: Physical*, 2008.
- [15] H. J. Park, et al., "Design of bi-directional and multi-channel miniaturized telemetry module for wireless endoscopy," in *Proc. 2nd Int. IEEE-EMBS Conf. Microtechnologies in Medicine and Biology*, 2002, pp. 273-276.
- [16] M. Kfourì, et al., "Toward a miniaturised wireless fluorescence-based diagnostic imaging system," *IEEE J. Selected Topics in Quantum Electronics*, vol. 14, Jan/Feb, 2008.
- [17] P. Valdastrì, A. Menciassi, P. Dario, "Transmission power requirements for novel ZigBee implants in the Gastrointestinal tract," *IEEE Trans. Biomedical Engineering*, Vol.55, June 2008.
- [18] S. Y. Shin, H. S. Park, and W. H. Kwon, "Mutual interference analysis of IEEE 802.15.4 and IEEE 802.11b," *Computer Networks*, vol. 51, August 2007, Pages 3338-3353.
- [19] VD6725, STMicroelectronics, <http://www.st.com/stonline/products/literature/bd/14370.pdf>, 2009.
- [20] Smallbattery. 2009. http://www.smallbattery.company.org.uk/hearing_aid_batteries.htm.
- [21] S. L. Jungles, "Wireless capsule endoscopy a diagnostic tool for early Crohn's Disease," *US Gastroenterology Review* 2005 - April 2005.
- [22] C. Kim, T. Lehmann, S. Nooshabadi and I. Nervat, "An ultra-wideband transceiver architecture for wireless endoscopes," *International Symp. Commun. and Information Tech.*, pp. 1252-1257, 2007.
- [23] T. Dissanayake, M. R. Yuçe and Ho C. K. "Design and evaluation of a compact antenna for implant-to-air UWB communication," *IEEE Antennas and Wireless Prop. Letters*, vol. 8, Page(s):153 - 156, 2009.
- [24] N. Aydin, T. Arslan, and D. R. S. Cumming, "Design and implementation of a spread spectrum based communication system for an ingestible capsule," *IEEE Trans. Information Technology in Biomedicine*, Vol.9, March 2005.
- [25] S. Mackay and B. Jacobson, "Endoradiosonde", *Natural*, vol. 179, pp.1239-1240, 1957.
- [26] www.google.nl/patents/US6632175.



10.22214/IJRASET



45.98



IMPACT FACTOR:
7.129



IMPACT FACTOR:
7.429



INTERNATIONAL JOURNAL FOR RESEARCH

IN APPLIED SCIENCE & ENGINEERING TECHNOLOGY

Call : 08813907089  (24*7 Support on Whatsapp)