



iJRASET

International Journal For Research in
Applied Science and Engineering Technology



INTERNATIONAL JOURNAL FOR RESEARCH

IN APPLIED SCIENCE & ENGINEERING TECHNOLOGY

Volume: 9 Issue: VI Month of publication: June 2021

DOI: <https://doi.org/10.22214/ijraset.2021.35435>

www.ijraset.com

Call:  08813907089

E-mail ID: ijraset@gmail.com

Automatic Detection of Mitral Regurgitation from Heart Sounds using SODP of Imperical Mode Decomposition

Gabbar Jadhav¹, Sagarika Yadav Jada², R. Triveni³, Mr. S. I. Khan⁴

^{1, 2, 3}Student, Sreenidhi Institute of Science and Technology, Ghatkesar, Telangana.

⁴Associate Professor, Sreenidhi Institute of Science and Technology, Ghatkesar, Telangana.

Abstract: *In this paper we discussed the heart valve disease. This heart valve disease occur throughout the world due to the more ethical estimation and grow curator of heart valve diseases use the diagnosis for this type of valve disease . Actually Phonocardiogram (PCG) signals are used because it having less price and acquire the signals. In this we learn five different kind of heart areas, Also typical are aortic stenosis, mitral valve prolapse, mitral stenosis and mitral regurgitation.*

Keywords: *phonocardiogram, diagnosis, aortic stenosis, mitral regurgitation.*

I. INTRODUCTION

One of the dangerous diseases is cardiovascular disease. Upon the globe more than 17 million members are there. Cardio vascular disease is the need of demised. It involves some state like pathological state of the heart, vessels of blood or valves of heart around of many diseases. This heart valve disease occur throughout the world due to the more ethical estimation and grow curator of heart valve diseases as compared with other Cardiovascular disease.

TTE is having less price and more observing time and it is benchmark for HVD diagnosis is transthoracic echocardiography .By acoustic window limitation image quality is degraded.

Heart valve illness has one or more valves in our heart, because we have the four valves in our heart. Blood is continuous to flow in the right direction in four valves. However, certain cases do not open or close one or more valves adequately since our blood flows through our hearts to destroy our bodies.

PhonoCardiogram is an acoustic wave recording produced by the mechanical action of the heart sound. It consists of two types of heart and cardiac mutations, acoustic vibration. Heart murmur is nothing more than symptoms of heart valve pathological alteration. In diagnosing heart disease it is important tool for acknowledging cardiac acculturation, but it is not enough for the diagnosis of some cardiac disease because it cannot be analysed to obtain qualitative as well as quantitative characteristics that are more costly and visual screening can take time to capture the signals, and the visual signals can be incorrect.

To overcome these limitations we use the artificial intelligence why we are using artificial intelligence because it having statistical analysis, feature selection and classification. In artificial intelligence techniques such as machine learning deep learning techniques are used. In Machine learning have take more time and subjective and some time error also take place. To overcome this Machine learning use deep learning techniques because it not require any characterstic like taking out, selecting and categorize.

Actually in deep learning concept we use the wave net architecture of the Phonocardiogram signals for categorize the sounds of heart in Heart valve disease.

II. LITERATURE REVIEW

Heart valve disease are occur due to damage of heart valve over time actually there having 4 valves that function is like one way gate the four heart valves are pulmonary, aortic, mitral and tricuspid valve.

In this 4 valves open and close properly and blood is flow properly through valves it having good mechanical heart. If there is any damage in one of the four then occur the heart valve disease.

Normally by using the stethoscope we listen the heart beat sounds. But we don't know exact functionality of heart sound that's why we are using the diagnosis process. One of the HVD diagnosis is TTE transthoracic echocardiography. This TTE having less price and observe time is more and quality of picture is worst.

Echocardiogram is a check that pumps blood through our heart's heart chambers and valves. It employs electrodes to assess the rhythm of your heart and sound technology in order to view blood moving through your heart. Diagnosis of cardiac problems.

III. METHODOLOGY


A EEG dataset which may be accessed online[27] is used in this investigation. The dataset comprises of 5 subsets with 100 EEG signal transmitters (Z, O, N, F, and S), each with 23.6 s. This data set consists of 5 subsets. For artefact visual evaluation from the continuous EEG multichannel recording these signals have been selected. The Z and O subsets were extracranially registered, while the N, F and S subsets were intracranially registered. Subsets Z and O were acquired with opened and closed eyes from the EEG surface of five healthy subjects. The signal was obtained in two groups in 5 patients (F subset) in the epileptogenic area and in the hippocampus of brain opposite hemisphere at seizure-free intervals (subset N). The S sub-set includes seizures, picked from all logging locations with ictal events. These partial convulsions are potentially complicated, which can eventually lead to secondary, widespread clonal convulsions. Sampled frequency of 173,61 Hz is the EEG signals in the datasets. Randomization of the signals in the recording site. The mounting is a general standard average. In Fig. 1, typical EEG signals are listed (one per subset). The results of this work unite the Z, O, N and F sub-sets with the NS class and S under the Seizur class.






IV. FUTURE WORK

First the patient is going to hospital and use sensor like stethoscope and by using data acquisition filter and amplify the signal and it convert the analog to digital converter and then preprocessing and segmentation takes place and signal is processing through feature extraction and selection by classify for medical diagnostic decision by the medical practitioners.

V. RESULTS

We received 97 percent of the classification of heart sounds into five categories. We were willing. For the usual class, the excessive precision category was 98,20 percent. The expansion type was confirmed by a 10-fold cross-validation, such protest and strength. To our best knowledge our study is the first to present a 5-degree cardiovascular classification study using the deep WaveNet model, following an intensive evaluation of deep models used to automate cardiovascular detection. Figure 5 shows the accuracy of the WaveNet model and stresses 97% of the accuracy of trainings. It is obvious that validation accuracy progressively increased from period 1 to 5, with minimal variation and a gradual improvement from stage 5, as the model symptomatically found an optimum solution. Figure 6 shows the pattern's confusion matrix. In the matrix it is to be noticed that the error rates in N, MVP, MS, MR and AS are 6%, 11%, 11% and 6% accordingly. The low error rate demonstrates how strong our technique is and how discriminating components are immediately removed.

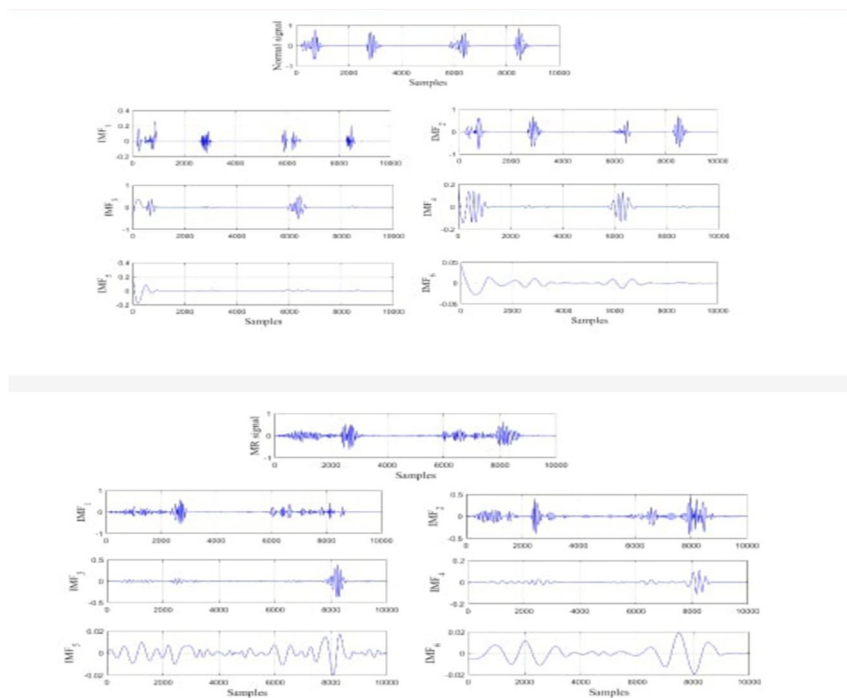

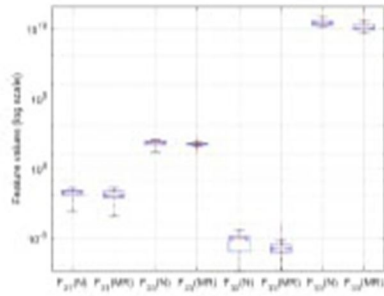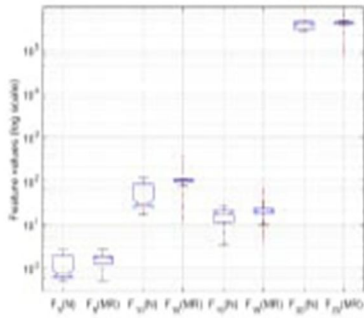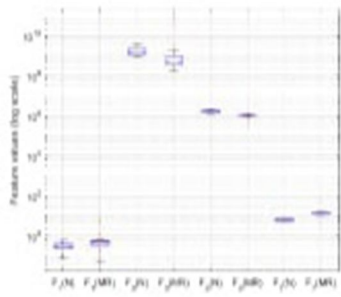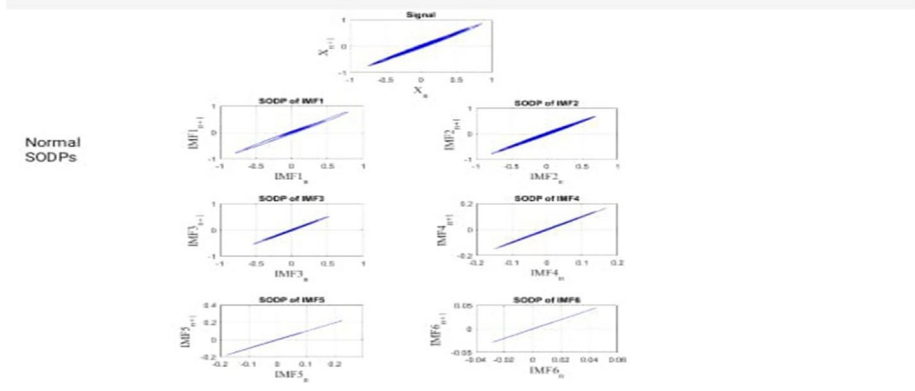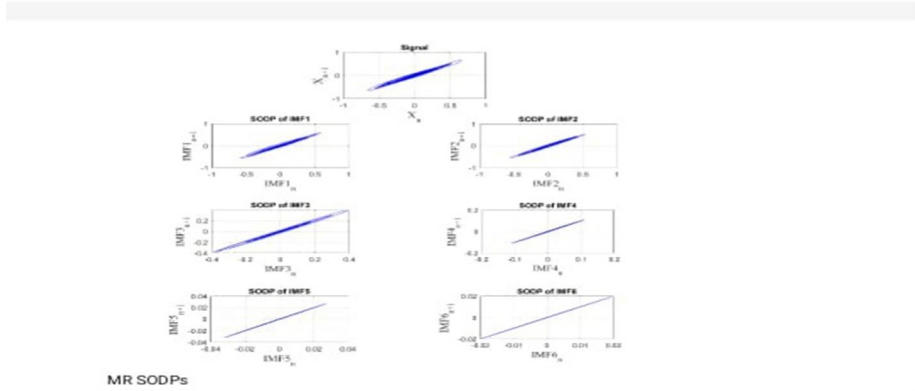

VI. CONCLUSION

In this paper We conclude that exact mark that the evolve type is categorize the five different types of the heart sound with error free . The advanced method can be employed in the discovery of cardiac illness in patients by specialists in the heart.

VII. ADVANTAGES

- A. The model is solid because it was used to record and check data ten times.
- B. The influence of atrocious convolutionary coverings can quickly instruct this type.
- C. The type can be instructed for a high quality of the data (in tens of thousands).

VIII. LIMITATIONS

- A. The type needs to be assembled and trained before categorization.
- B. WaveNet is a large model that requires a large storage capacity, and can therefore cost computationally.

REFERENCES

- [1] "Cardiovascular diseases, CVD Fact Sheet," World Health Organisation. .
- [2] T. Vos et al., "Global, regional, and national incidence, prevalence, and years lived with disability for 301 acute and chronic diseases and injuries in 188 countries, 1990-2013: A systematic analysis for the Global Burden of Disease Study 2013," *Lancet*, 2015.
- [3] D. Mozaffarian et al., "Executive summary: Heart disease and stroke statistics-2016 update: A Report from the American Heart Association," *Circulation*, vol. 133, no. 4, pp.447-454, 2016.
- [4] J. Draper, S. Subbiah, R. Bailey, and J. B. Chambers, "Murmur clinic : validation of a new model for detecting heart valve disease," pp. 56-59, 2019.
- [5] J. P. Dominguez-Morales, A. F. Jimenez-Fernandez, M. J. Dominguez-Morales, and G. Jimenez-Moreno, "Deep Neural Networks for the Recognition and Classification of Heart Murmurs Using Neuromorphic Auditory Sensors," *IEEE Trans. Biomed. Circuits Syst.*, vol.12, no. 1, pp. 24-34, 2018.
- [6] O. Faust, R. Acharya U, S. M. Krishnan, and L. C. Min, "Analysis of cardiac signals using spatial filling index and time-frequency domain," *Biomed. Eng. Online*, vol. 3, pp. 1-11, 2004.
- [7] Yaseen, G. Y. Son, and S. Kwon, "Classification of heart sound signal using multiple features," *Appl. Sci.*, vol. 8, no. 12, 2018.
- [8] S. Patidar and R. B. Pachori, "Classification of cardiac sound signals using constrained tunable-Q wavelet transform," *Expert Syst. Appl.*, vol. 41, no. 16, pp. 7161-7170, 2014.
- [9] S. Ari, K. Hembram, and G. Saha, "Detection of cardiac abnormality from PCG signal using LMS based least square SVM classifier," *Expert Syst. Appl.*, vol. 37, no. 12, pp. 8019-8026, 2010.
- [10] J. Li, L. Ke, and Q. Du, "Classification of Heart Sounds Based on the Wavelet," *Entropy*, vol. 21, no. 5, p. 472, 2019.
- [11] F. Safara, S. Doraisamy, A. Azman, A. Jantan, and A. R. Abdullah Ramaiah, "Multi-levelbasis selection of wavelet packet decomposition tree for heart sound classification," *Comput. Biol. Med.*, vol. 43, no. 10, pp. 1407-1414, 2013.
- [12] Y. Zheng, X. Guo, and X. Ding, "A novel hybrid energy fraction and entropy-based approach for systolic heart murmurs identification," *Expert Syst. Appl.*, vol. 42, no. 5, pp.2710-2721, 2015.
- [13] S. K. Randhawa and M. Singh, "Classification of Heart Sound Signals Using Multi-modal Features," *Procedia Comput. Sci.*, vol. 58, pp. 165-171, 2015.
- [14] S. K. Ghosh, R. N. Ponnalagu, R. K. Tripathy, and U. R. Acharya, "Automated detection of heart valve diseases using chirplet transform and multiclass composite classifier with PCG signals," *Comput. Biol. Med.*, vol. 118, no. February, 2020.
- [15] C. Xu, Q. Long, and J. Zhou, "S1 and S2 heart sound recognition using optimized BP neural network," *ACM Int. Conf. Proceeding Ser.*, vol. 64, no. 2, pp. 105-110, 2019.
- [16] V. Maknickas and A. Maknickas, "Recognition of normal-abnormal phonocardiographic signals using deep convolutional neural networks and mel-frequency spectral coefficients," *Physiol. Meas.*, vol. 38, no. 8, pp. 1671-1684, 2017.
- [17] E. Kay and A. Agarwal, "DropConnected neural networks trained on time-frequency and inter-beat features for classifying heart sounds," *Physiol. Meas.*, vol. 38, no. 8, pp. 1645-1657, 2017.
- [18] C. Potes, S. Parvaneh, A. Rahman, and B. Conroy, "Ensemble of feature-based and deep learning-based classifiers for detection of abnormal heart sounds," *Comput. Cardiol. (2010).*, vol. 43, no. December, pp. 621-624, 2016.
- [19] M. Tschannen, T. Kramer, G. Marti, M. Heinzmann, and T. Wiatowski, "Heart sound classification using deep structured features," in *2016 Computing in Cardiology Conference (CinC)*, 2016, pp. 565-568.
- [20] M. J. Legato, "Gender and the heart: sex-specific differences in normal anatomy and physiology.," *The journal of gender-specific medicine: JGSM : the official journal of the Partnership for Women's Health at Columbia*. 2000.



10.22214/IJRASET



45.98



IMPACT FACTOR:
7.129



IMPACT FACTOR:
7.429



INTERNATIONAL JOURNAL FOR RESEARCH

IN APPLIED SCIENCE & ENGINEERING TECHNOLOGY

Call : 08813907089  (24*7 Support on Whatsapp)