



IJRASET

International Journal For Research in
Applied Science and Engineering Technology



INTERNATIONAL JOURNAL FOR RESEARCH

IN APPLIED SCIENCE & ENGINEERING TECHNOLOGY

Volume: 9 Issue: VII Month of publication: July 2021

DOI: <https://doi.org/10.22214/ijraset.2021.36478>

www.ijraset.com

Call:  08813907089

E-mail ID: ijraset@gmail.com

Design and Development of a Smart Seat for Relieving from Pressure Ulcers

Er. Rohit Tembhurne¹, Dr. Shubhangi Giripunje²

^{1,2}Department of Electronics & Telecommunication, RTMNU University, Nagpur, Maharashtra, India

Abstract: *The long-term effects of sitting in a wheelchair/chair can be painful. People who use wheelchairs/chair can get muscle deformities and even serious injuries. Wheelchair/chair injuries and pains, such as pressure ulcers, normally hit people who spend a significant amount of time in wheelchairs. Bad posture is another major challenge for people who use wheelchairs/chair because they are not able to change their sitting position.*

Keywords: *Pressure ulcers, cushion, load cell, body weight, air pressure, spinal cord injury*

I. INTRODUCTION

A pressure ulcer is an area of skin that breaks down when something keeps pressing or rubbing against the skin. It is a localized injury to the skin and its underlying tissue, usually over a bony prominence. Older people are at high risk of developing pressure ulcers due to their decreased physical and functional health conditions, which lead to decreased mobility and confinement to chair or bed. Over 50% of pressure ulcers are around the sitting areas near to the buttocks. In the early stage, the formation of pressure ulcers can be avoided by the application of appropriate treatment and preventive measures such as special pressure relieving seat cushions. Sitting for prolonged periods of time is thought to increase the risk of developing pressure ulcers. Sitting forces the weight of an individual against the supporting seat surface which compresses the soft tissues around the buttock area between the chair and the bony ischial tuberosities. This pressure causes an obstruction of blood flow that when combined with limited movement, poor sensation, malnutrition, and increased age can eventually lead to ulceration. These severe, yet usually preventable wounds are relatively common, spanning acute, rehabilitation, and community settings, as such, the treatment of pressure ulcers is considered to outweigh the social and financial costs associated with prevention.

One of the most effective preventative methods in terms of cost and pressure relief is regular repositioning. Within rehabilitation, individuals at risk of developing pressure ulcers are taught and encouraged to perform regular repositioning movements in order to redistribute the build-up of pressure around the ischial tuberosity and sacral regions. These repositioning movements include vertical pushups, lateral and forward leans. Occupational therapists being responsible for seating and postural care are ideally placed to educate the individual and their carers on good skin health and the importance of relieving pressure at the seating interface regularly.

II. OBJECTIVES

The objective of this project is design and development of a smart seat to provide a relief from the pressure ulcers to the patient and Relief the pressure of hip bones of the person on seating continuously for work.

III. METHODOLOGY

The work is discussed in four parts.

- A. Measure Weight Using Load Cell And Pass To The Controller
- B. Connect the air pump to fill air into cushion
- C. Connect solenoid to realising pressure
- D. Test on adjusting surface pressure using switches

The first part is concerned with the construction of a state-of-the-art pressure sensor, as well as a color LCD screen displaying the pressure distribution with the use of an Arduino Nano microcontroller.

Next, fill air into cushion according to weight, Various sitting postures and seat materials are used to test their impact on the sitting pressure distribution. Sitting postures include normal position and leaning forward.

The third part is on the connection on solenoid valve opens up to release the air.

The forth part is connect the switches for add pressure and release the air manually.

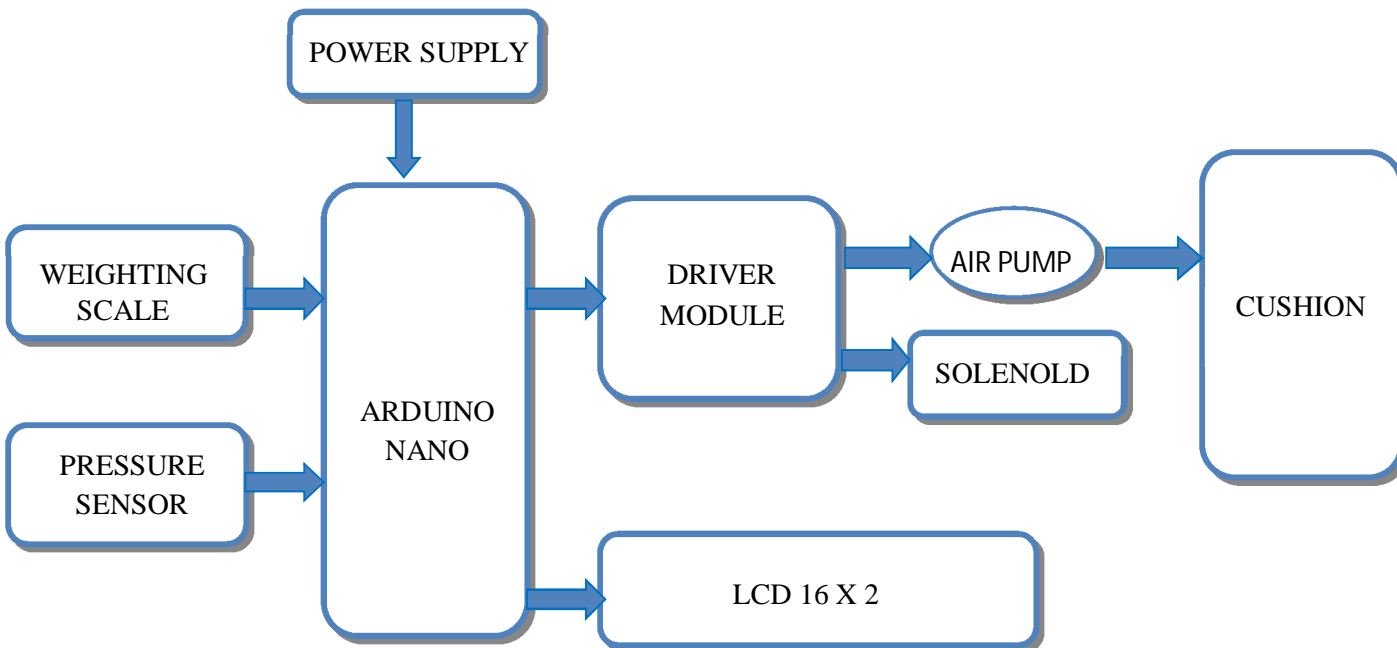


Fig1. Block Diagram A Smart Seat For Relieving From Pressure Ulcers

IV. SCHEMATIC ARRANGEMENT

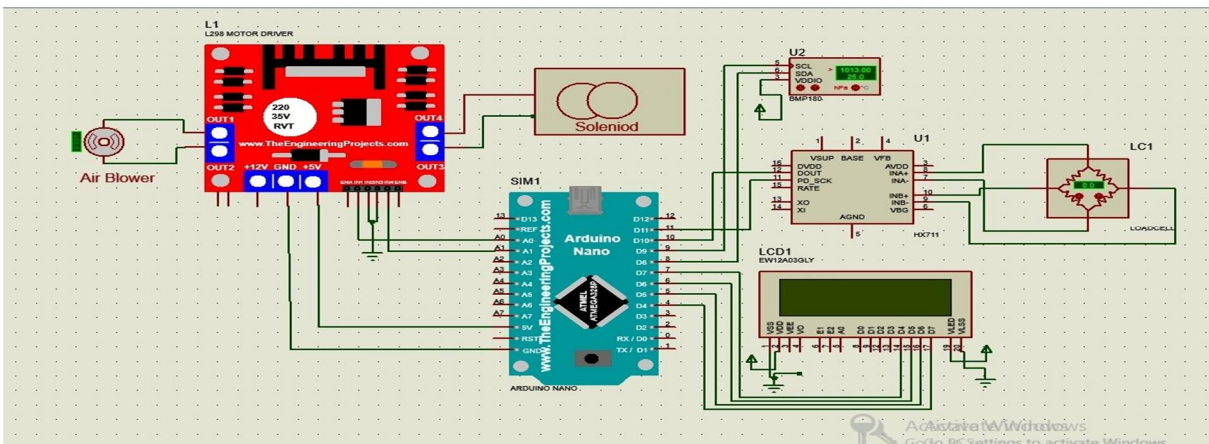


Fig2. Schematic Diagram

V. WORKING OF PROJECT

We are designing a system which will improve sitting arrangement for peoples. It is weight based cushion air pressure controlling system.

We will fill the air pressure in cushion according to weight of user.

Proposed system has arduino as a microcontroller board which used to control all the peripheral devices. A pressure sensor to measure air presser in air cushion. An air pump to fill air in cushion, a solenoid valve to release the air pressure.

To measure weight of a person we have weighing scale and lcd to show weight and pressure.

We used driver module L298 to drive air pump and solenoid.

12Volt 2Amp power supply is used for the project. On powering up the supply, Controller will initialize all sensors and actuators along with lcd display. After this controller will wait for the person to measure the weight.

After getting weight controller decide the air pressure to be filled in cushion. As soon as the weight is measure air realising solenoid valve opens up to release the air. It will be opened for 3 sec. as it is sufficient to release the pressure.

Once release, air pump started filling air with showing current pressure on LCD. Air pressure sensor reads the air pressure inside the cushion. Once the air pressure reaches the calculated pressure air pump stops the air flow. This is how we automate the process the blowing air inside cushion according to the weight.

We also have option to increase or decrease air pressure using manual push buttons.

VI. HARDWARE IMPLEMENTATION

A. Components Required To Smart Seat, The Required Components Are Listed Below

- 1) Air Pump
- 2) L298 Motor driver module
- 3) Solenoid Valve
- 4) Power supply
- 5) Arduino Nano
- 6) Cushion
- 7) Load Cell
- 8) LCD Display
- 9) Connectors and Cables

B. Mechanical Body Description

- 1) Mount All The Component on the wood board and connect air pump , solenoid valve and LCD display through L298 Motor Driver to arduino nano

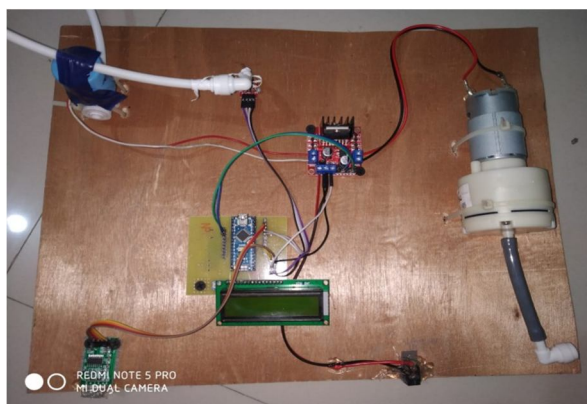


Fig3. Mount Component On Wood Board

- 2) Connect Air Pump to cushion for fill air through pipe



Fig4. Connect Air Pump

3) Connect Solenoid Valve to cushion for realising air through pipe

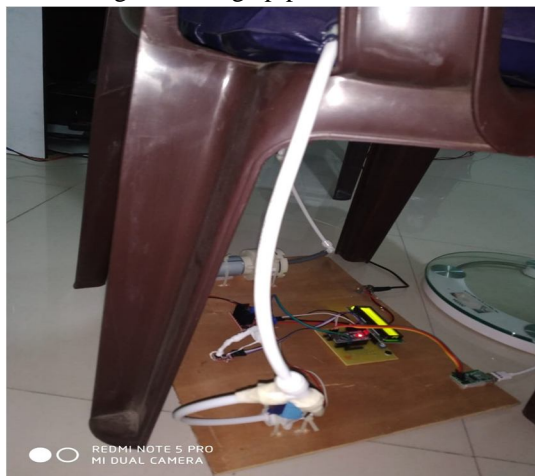


Fig5. Connect Solenoid Valve

4) Show Weight And Pressure in LCD Display

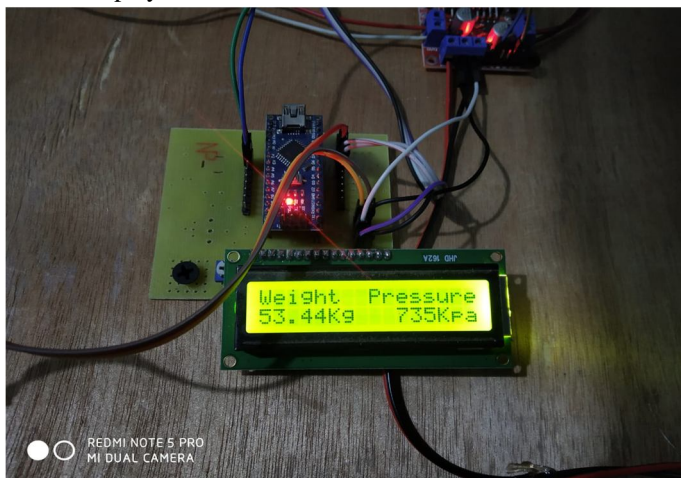


Fig6. Show Weight And Pressure on LCD Display

5) Complete Smart Seat



Fig6. Complete Smart Seat

VII. APPLICATION

It will be helpful in following applications:

- A. For connecting rural area patients with specialized doctors.
- B. Use By hospitals.
- C. Used For Ulcers Patient.
- D. Used For Office Employees.

VIII. CONCLUSION

The goal of WCM development described in this paper was to provide wheelchair bound SCI patients with a pressure monitoring system that can aid in the prevention of pressure ulcers. Potentially, this affordable device may improve the life of individuals with SCI, as it alerts patients and/or caregivers in the events of pressure hazards. The initial prototype of the device demonstrates technical feasibility of implementing WCM as an accurate, low-cost and low-power, always-on device for monitoring of air-filled wheelchair cushions. Further

work on the device will include further extension of its functionality and formal testing in human studies.

The goal of WCM development described in this paper was to provide wheelchair bound SCI patients with a pressure monitoring system that can aid in the prevention of pressure ulcers. Potentially, this affordable device may improve the life of individuals with SCI, as it alerts patients and/or caregivers in the events of pressure hazards. The initial prototype of the device demonstrates technical feasibility of implementing WCM as an accurate, low-cost and low-power, always-on device for monitoring of air-filled wheelchair cushions. Further work on the device will include further extension of its

functionality and formal testing in human studies. The goal of WCM development described in this paper was to provide wheelchair bound SCI patients with a pressure monitoring system that can aid in the prevention of pressure ulcers. Potentially, this affordable device may improve the life of individuals with SCI, as it alerts patients and/or caregivers in the events of pressure hazards. The initial prototype of the device demonstrates technical feasibility of implementing WCM as an accurate, low-cost and low-power, always-on device for monitoring of air-filled wheelchair cushions. Further work on the device will include further extension of its functionality and formal testing in human studies.

The goal of smart seat development described in this paper was to provide chair bound SCI patients with a pressure monitoring system that can aid in the prevention of pressure ulcers. Potentially, this affordable device may improve the life of individuals with SCI, as it alerts patients and/or caregivers in the events of pressure hazards. The initial prototype of the device demonstrates technical feasibility of implementing smart seat as an accurate, low-cost and low-power, always-on device for monitoring of air-filled chair cushions. Further work on the device will include further extension of its functionality and formal testing in human studies.

REFERENCES

- [1] Catia Tavares, M. Fatima Domingues, Tiago Paixao, Nelia Alberto, Wheelchair Pressure Ulcer Prevention Using FBG Based Sensing Devices. MDPI and ACS Style 30 December 2019.
- [2] Kwong, EWY, Hung M, and Woo K (2016). Improvement of pressure ulcer prevention care in private for-profit residential care homes: An action research study. BMC Geriatrics, 16: 192.
- [3] Alison Porter-Armstrong and may Stinson. Reviewing the Literature on the Effectiveness of Pressure Relieving Movements. Hindawi Publishing Corporation Nursing Research and practice. Article ID 124095. Published 13 Jan 2013.
- [4] Kwong EWY, Lau A, Lee R, Kwan R (2011). A pressure ulcer prevention programme specially designed for nursing homes: does it work?" Journal Clinical Nursing, 20(19-20), 2777-2786.
- [5] K. Vanderwee, M. H. F. Grypdonck, D. De Bacquer, and T. Defloor, "Effectiveness of turning with unequal time intervals on the incidence of pressure ulcer lesions," Journal of Advanced Nursing, vol. 57, no. 1, pp. 59-68, 2007.
- [6] A. Gefen, "The biomechanics of sitting-acquired pressure ulcers in patients with spinal cord injury or lesions," International Wound Journal, vol. 4, no. 3, pp. 222-236, 2007.
- [7] T. Ergic, Z. Ivandic and D. Kozak. "The Significance of Contact Pressure Distribution on The Soft Tissue by Men sitting", International Design Conference Design 2002. Dubrovnik. Croatia. May 2002.
- [8] Arduino open-source electronic prototyping platform, <https://www.arduino.cc/>.



10.22214/IJRASET



45.98



IMPACT FACTOR:
7.129



IMPACT FACTOR:
7.429



INTERNATIONAL JOURNAL FOR RESEARCH

IN APPLIED SCIENCE & ENGINEERING TECHNOLOGY

Call : 08813907089  (24*7 Support on Whatsapp)